

Figure 1

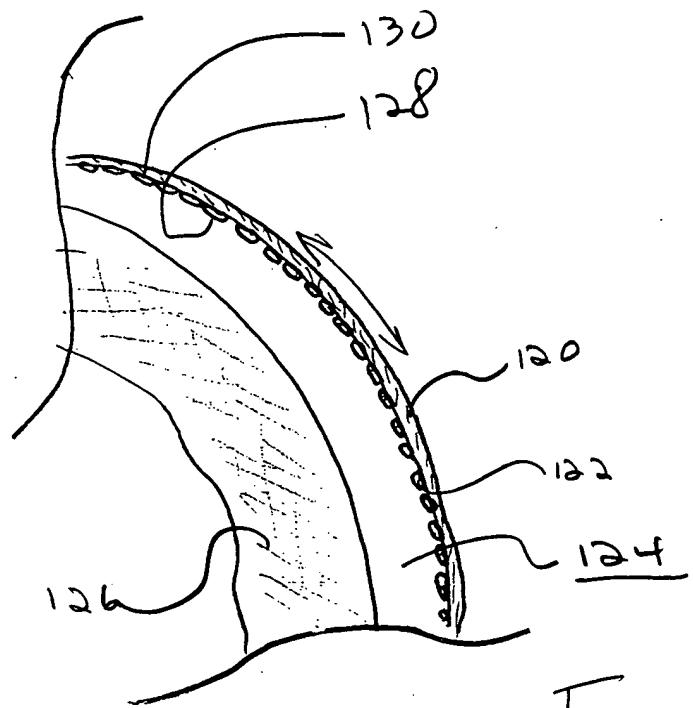


Figure 2

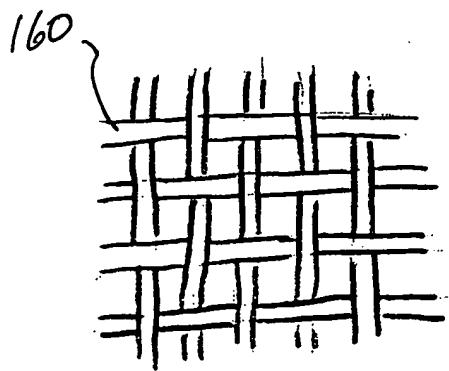
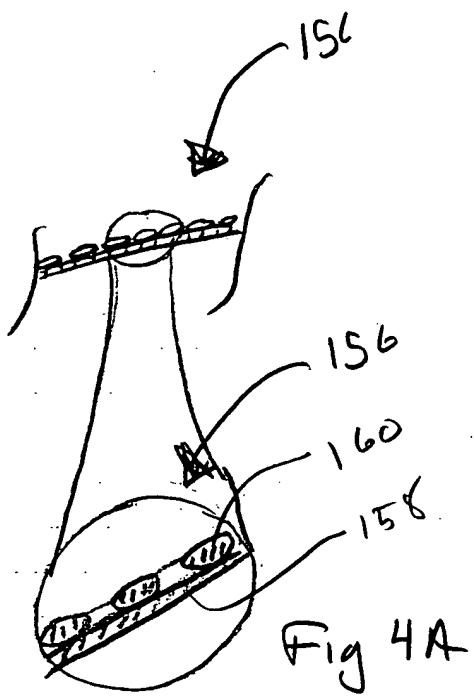
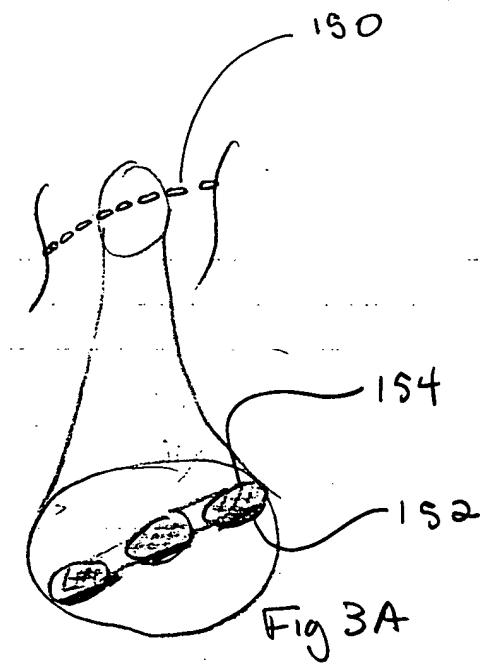
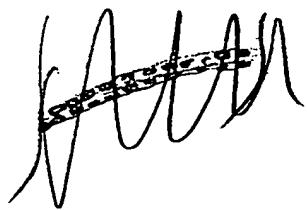



Fig 3B

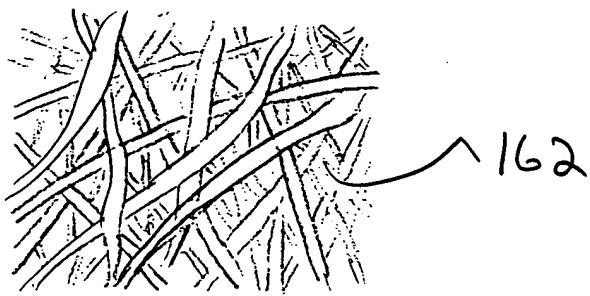
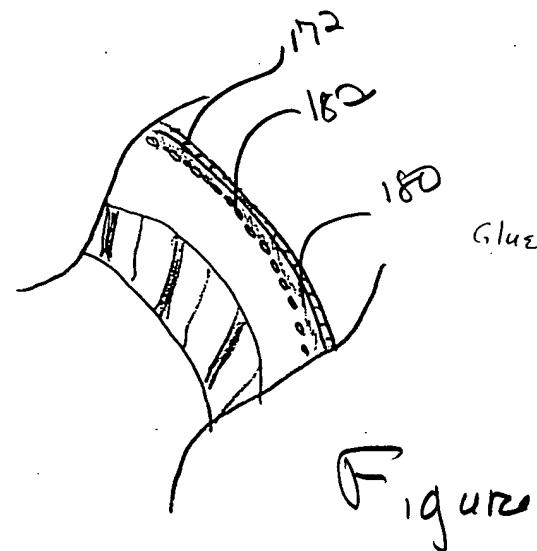
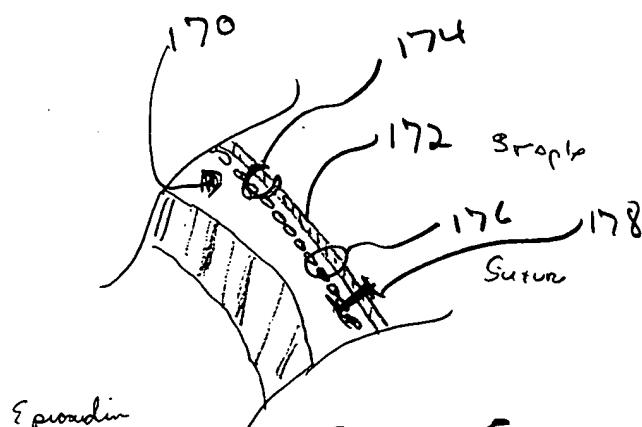
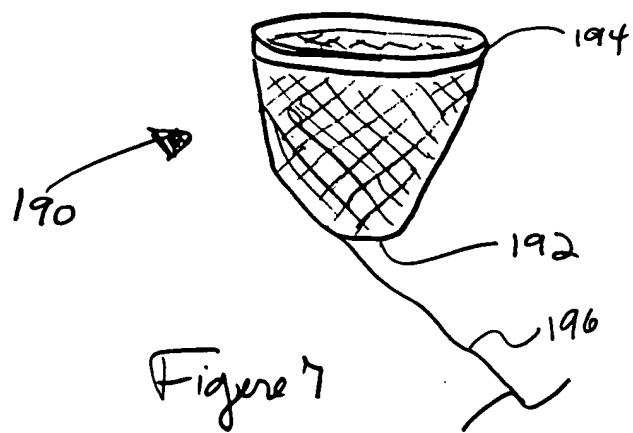
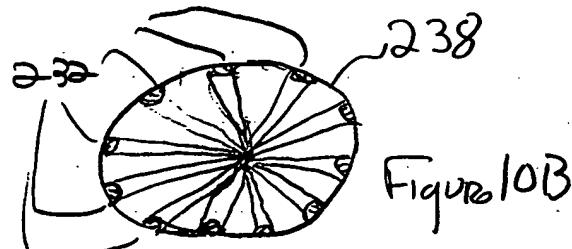
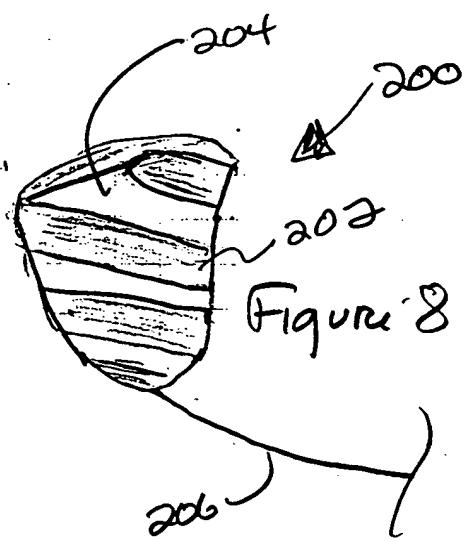
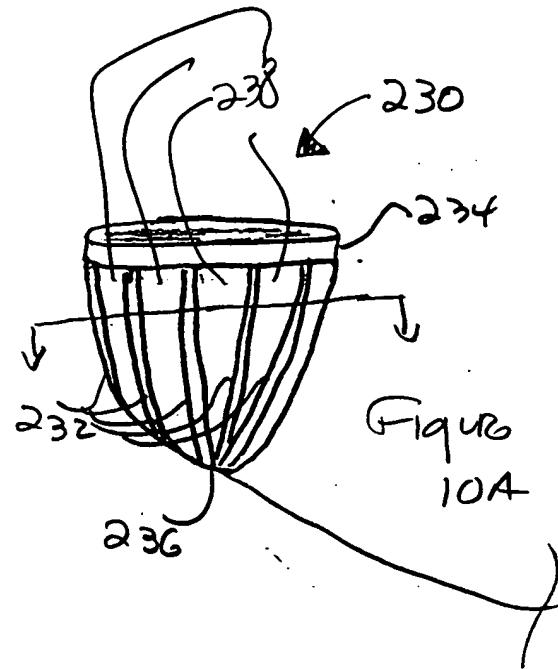
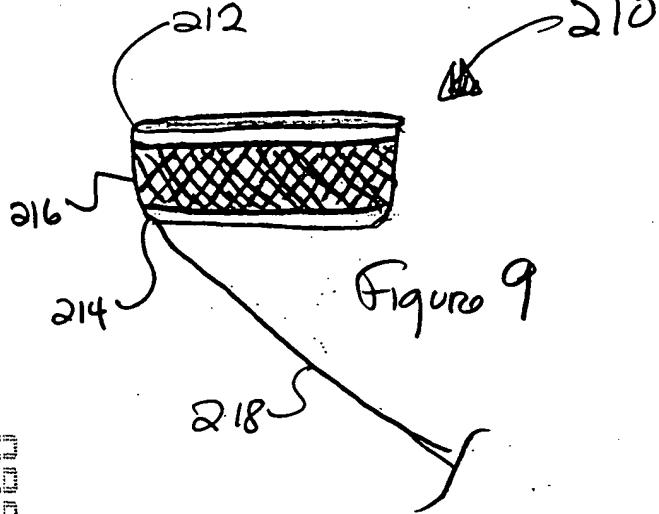
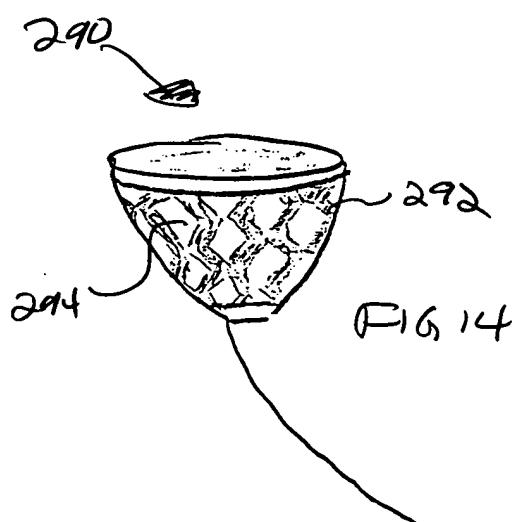
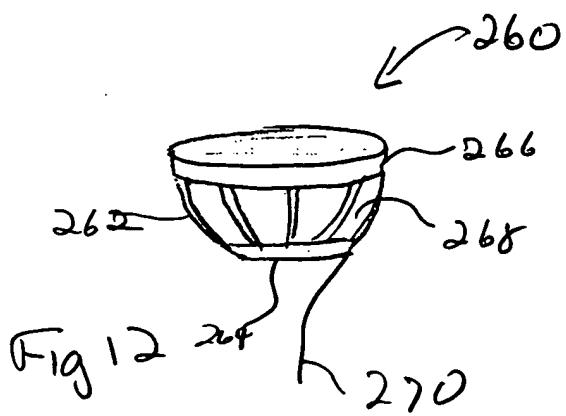
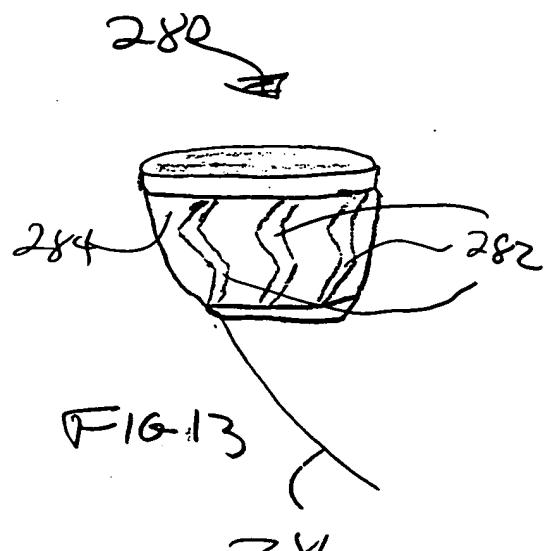
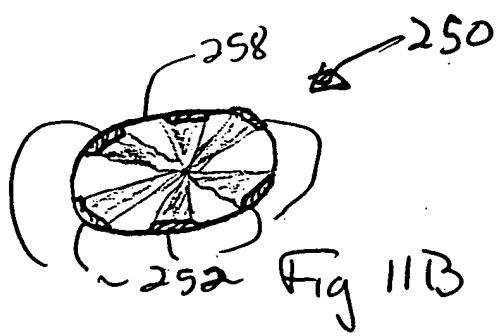
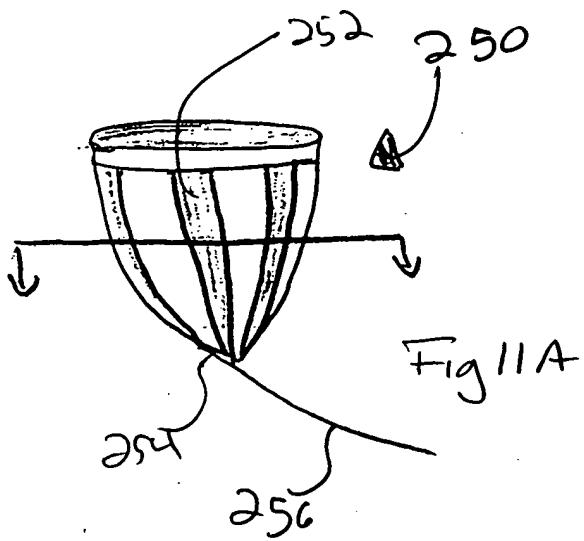
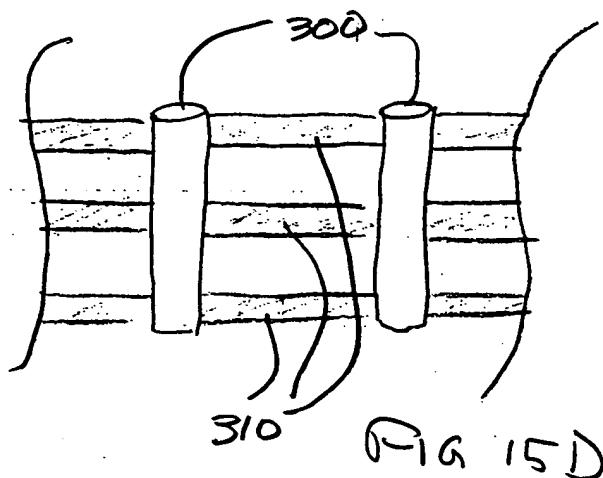
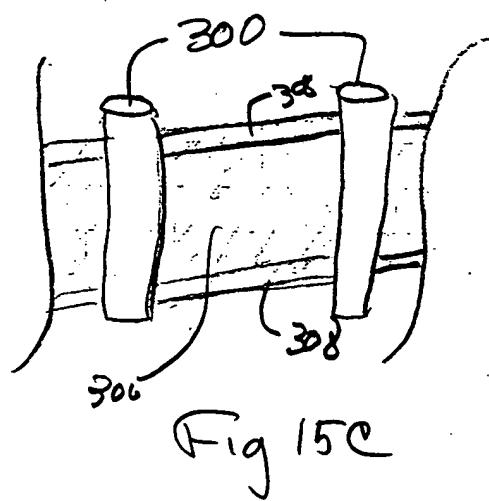
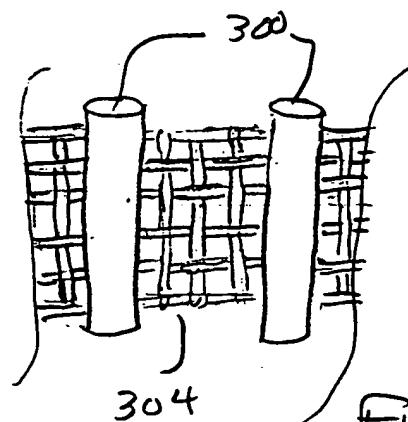
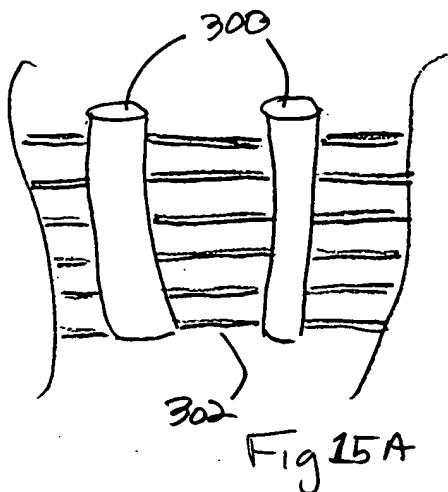




Fig 4B









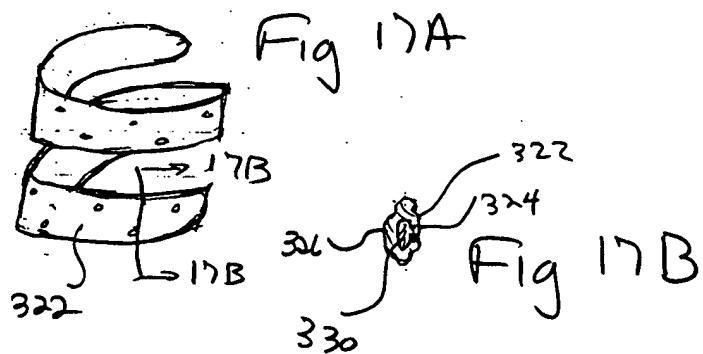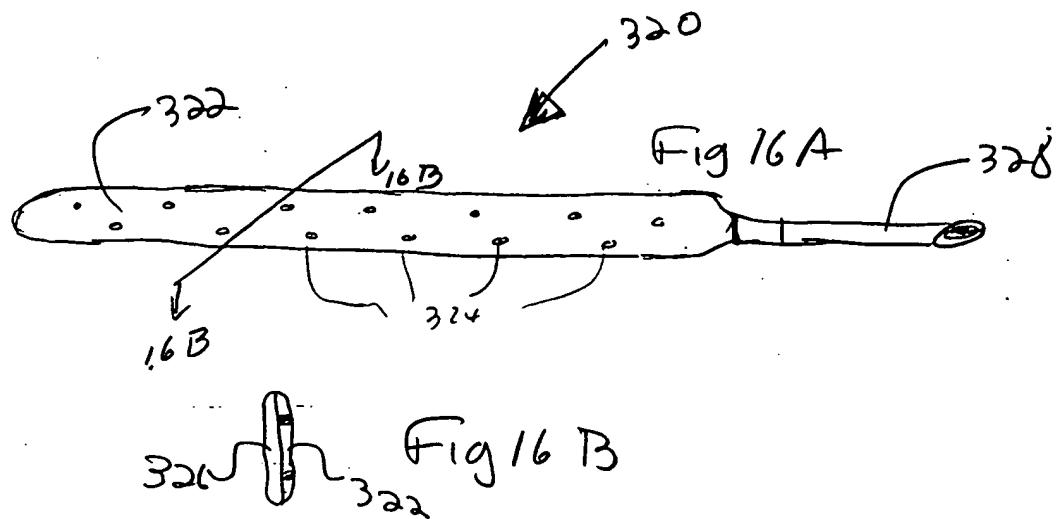

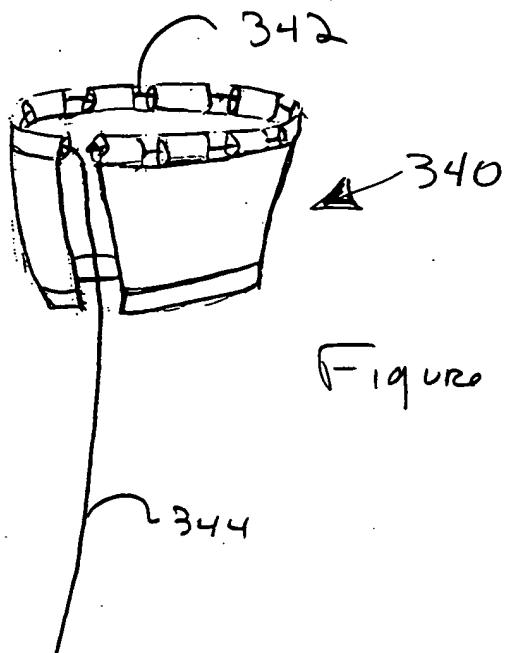


Figure 18

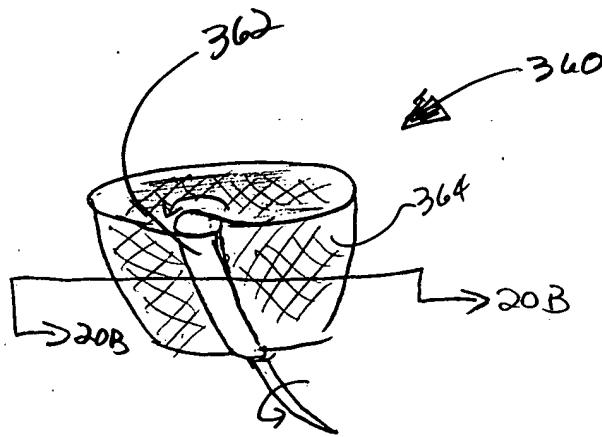
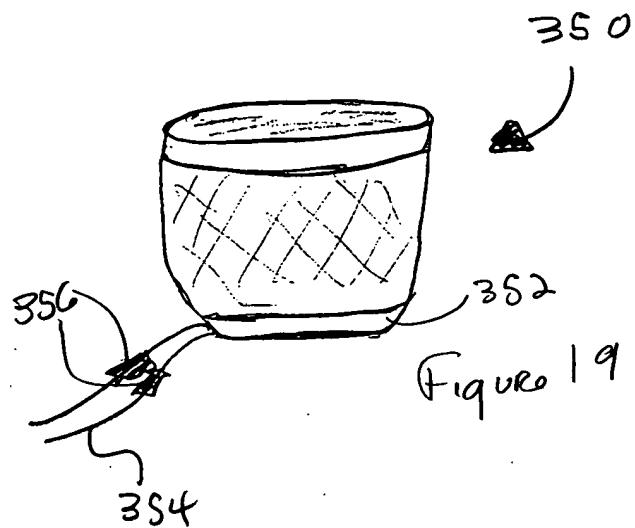
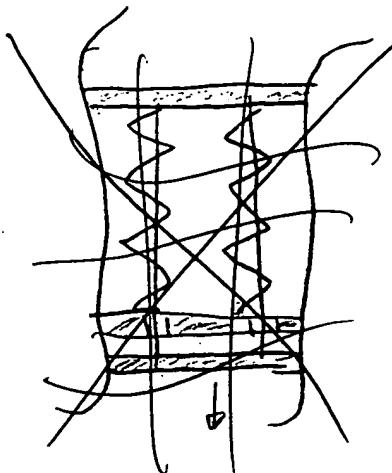


Figure 20A

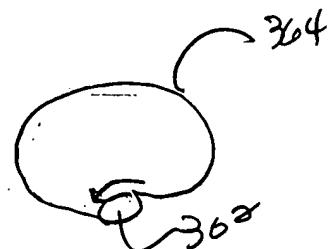


Figure 20B

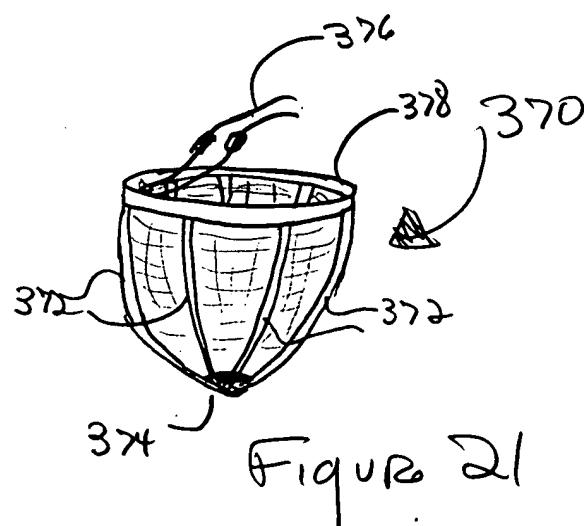


Figure 21

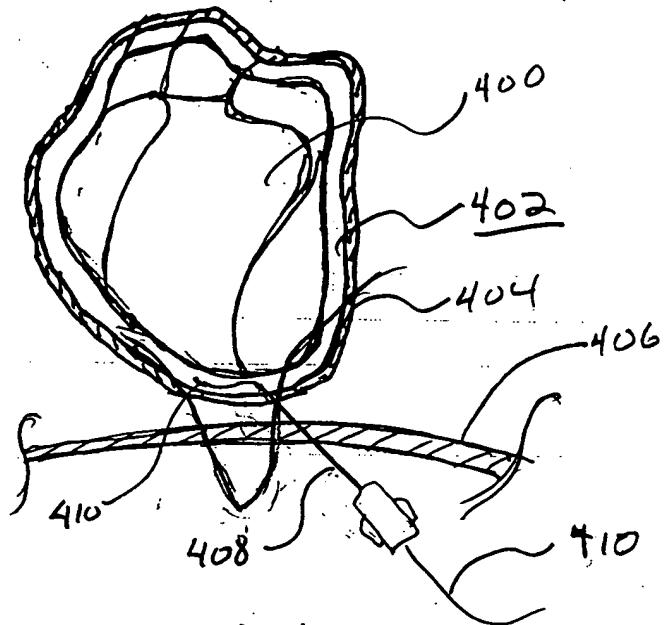


Figure 22 A

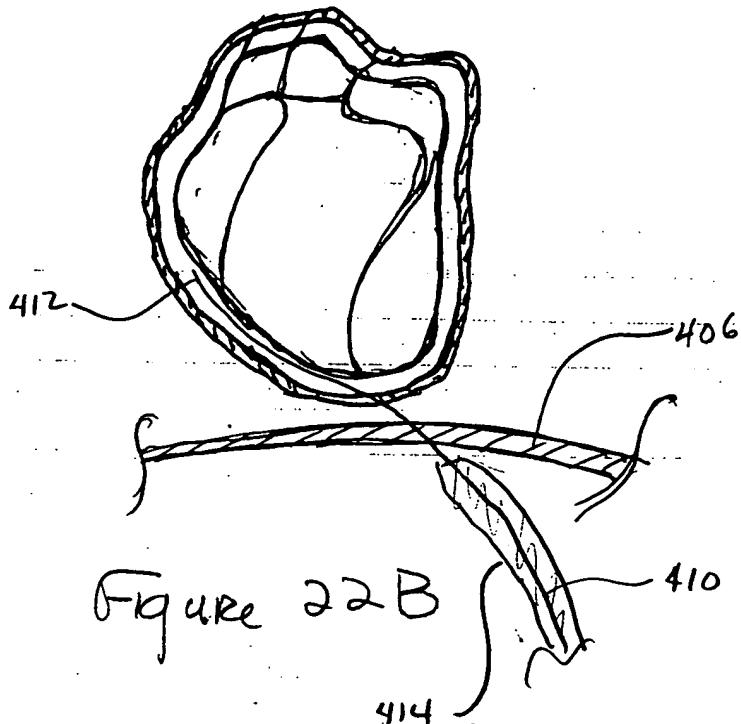
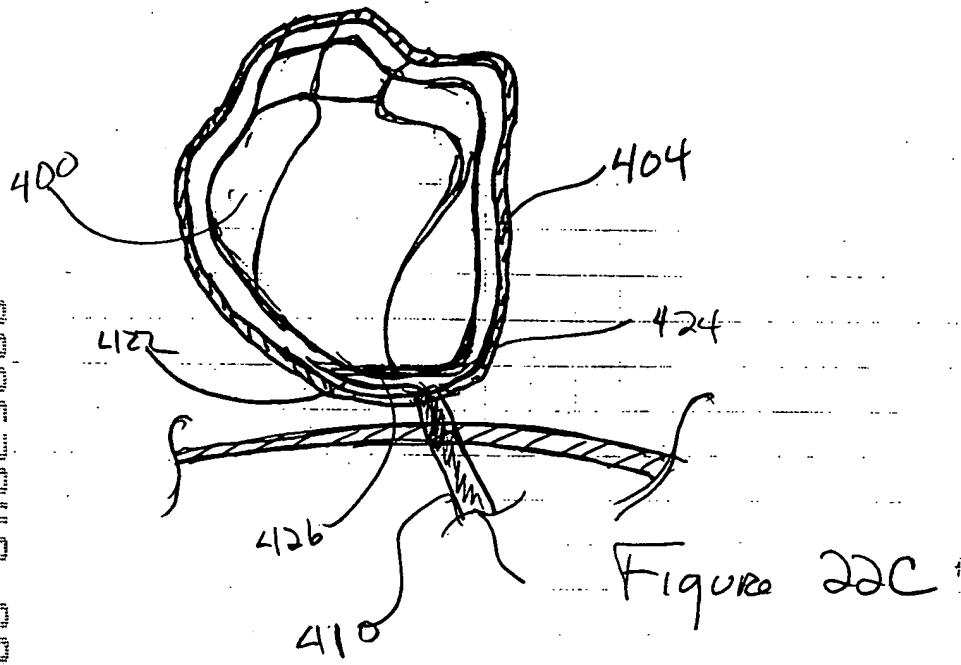


Figure 22B



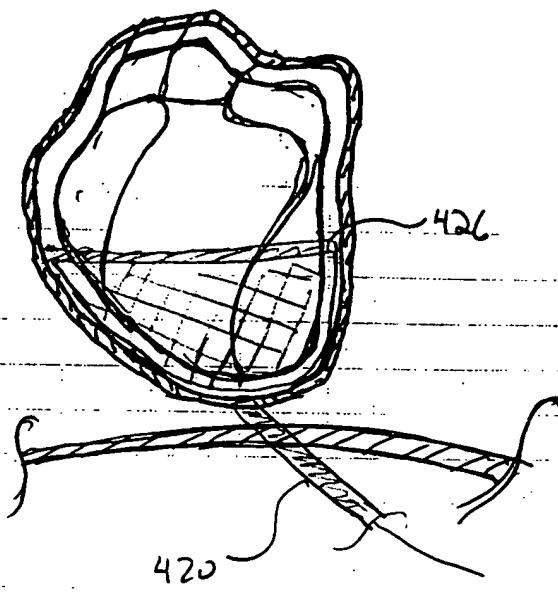


Fig 22D

Short Title: PERICARDIUM REINFORCING DEVICES AND
METHODS OF USING THEM
First Inventor: Ronald G. FRENCH et al.
Application No.: To Be Assigned
Docket No.: 509152000500

Sheet 15 of 15

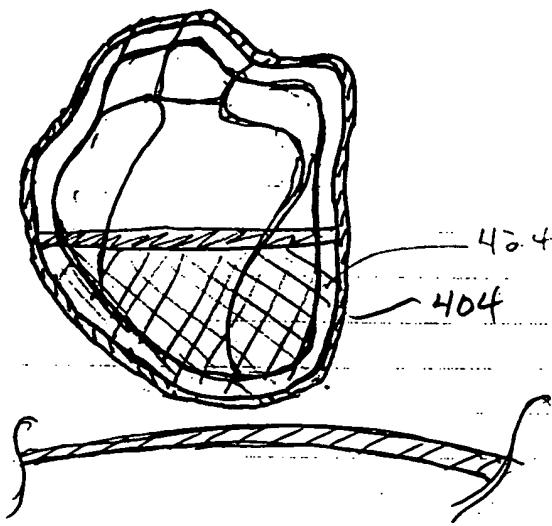


Fig 22 E

**This Page Is Inserted by IFW Operations
and is not a part of the Official Record**

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

**As rescanning documents *will not* correct images,
please do not report the images to the
Image Problem Mailbox.**